

## What's NEXT?

The Nationwide Evaluation of X-Ray Trends (NEXT) is a national program conducted annually to measure the x-ray exposure that a standard patient receives for selected x-ray examinations. This program is conducted jointly by the Conference of Radiation Control Program Directors (CRCPD), an association of state and local radiation control agencies, and the Food and Drug Administration's (FDA) Center for Devices and Radiological Health (CDRH).

In 1992 the selected examination was mammography, an examination which had previously been surveyed in 1985<sup>1</sup> and 1988<sup>2</sup>. Breast exposures were measured using each facility's technique for the craniocaudal (CC) view using a standard reference imaging phantom which approximates a 4.2 cm compressed breast for screen-film radiography. (4.7 cm compressed breast for xeroradiography.) The breast is assumed to be a 50/50% glandular/adipose tissue composition.

The data is presented only for screen-film mammography with grid as there are now an insufficient number of facilities performing xeromammography or S/F mammography without a grid to be statistically significant. Each set of data provides information on the entrance skin exposure (ESE) and half-value layer (HVL). From these data the mean glandular tissue dose was calculated.<sup>3</sup> Radiographs were obtained using a CDRH phantom which was equivalent in thickness to the phantom used by the American College of Radiology in their accreditation program. The radiographs were evaluated and given an image quality score. Surveys were performed by CDRH-trained participating state radiation control personnel.

*The information contained herein is for guidance. The implementation and use of the information and recommendations are at the discretion of the user. The mention of commercial products, their sources, or their use in connection with material reported is not to be construed as either an actual or implied endorsement by CRCPD or CDRH.*

<sup>1</sup>Nationwide Evaluation of X-Ray Trends (NEXT). Tabulation and Graphical Summary of Surveys 1984-1987. Conference of Radiation Control Program Directors, Frankfort, KY, CRCPD Pub. 89-3.

<sup>2</sup>Nationwide Evaluation of X-Ray Trends (NEXT). Tabulation and Graphical Summary of Survey for 1988. CRCPD Pub. 90-7.

<sup>3</sup>Handbook of Glandular Tissue Doses in Mammography, HHS Publication FDA 85-8239, March, 1985.

## SURVEY RESULTS

### Your Facility

|  |       |
|--|-------|
| Target                                   | _____ |
| Filter                                   | _____ |
| HVL (mm Al)                              | _____ |
| Mean glandular dose (mRad)               | _____ |
| Processing cycle (Std/Ext)               | _____ |
| Processing speed STEP* test result       | _____ |
| (refer to inside for recommended range)  |       |
| Phantom image score<br>( )= ACR min pass |       |
| fibers (4)                               | _____ |
| specks (3)                               | _____ |
| masses (3)                               | _____ |

\* Sensitometric Technique for the Evaluation of Processing

CRCPD  
1030 Burlington Lane, Suite 4B  
Frankfort, KY 40601  
www.crcpd.org

# Nationwide Evaluation of X-Ray Trends

## (NEXT)

## 1992 Mammography X-Ray Data

Conference of Radiation  
Control Program Directors


and

The Center for Devices and  
Radiological Health

U.S. DEPARTMENT OF HEALTH  
AND HUMAN SERVICES  
Public Health Service  
Food and Drug Administration

# 1992 NEXT Mammography Survey Results

## Processing Speed

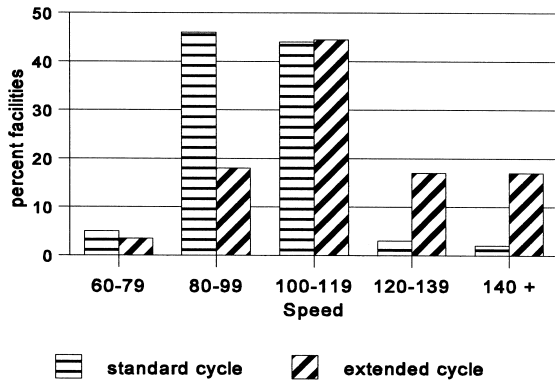

**Normal Processing\***: std= 80-120 Ext= 100 - 170  
 \* MQSA limits for normal processing.

## Processing : Percent Facilities by Cycle

| cycle | under | normal | over |
|-------|-------|--------|------|
| std   | 4.7   | 90.5   | 4.8  |
| ext   | 21.7  | 77.1   | 1.2  |


## Statistical Evaluation of Mammographic Parameters

|         | Mean Glandular Dose (mGy)* | Kilovoltage (kVp) | HVL (mm Al) |
|---------|----------------------------|-------------------|-------------|
| Mean    | 1.50                       | 27                | 0.35        |
| Std dev | 0.56                       | 1.4               | 0.05        |
| min     | 0.43                       | 20                | 0.17        |
| max     | 4.64                       | 32                | 0.71        |
| N       | 331                        | 342               | 336         |


\* note: 1 mGy = 100 mRad

# 1992 NEXT Mammography Survey Results

## HVL (mm Al)

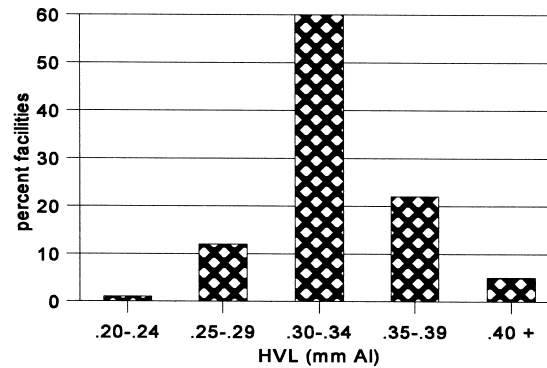


## kVp

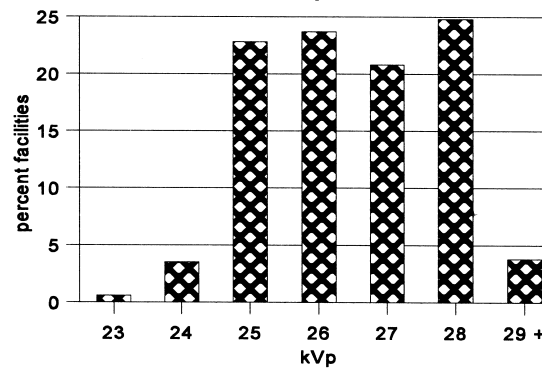

## Mean Glandular Dose\* (mGy)

\* 1 mGy = 100 mRad

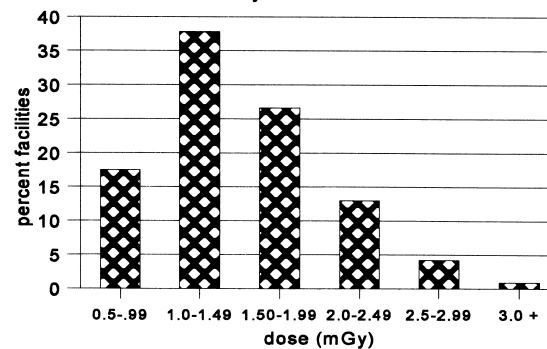

# 1992 NEXT Mammography Survey Results

## Comparison of 1992 NEXT with 1995 MQSA inspection results<sup>1</sup>

|                               | 1992 NEXT | 1995 MQSA |
|-------------------------------|-----------|-----------|
| Mean entrance skin exp (mR)   | 790       | 910       |
| Mean kVp                      | 27        | 26        |
| Mean HVL (mm Al) **           | 0.35      | 0.32      |
| Mean glandular dose * (mGy)   | 1.40      | 1.50      |
| Mean processing - std cycle   | 98        | 97        |
| Mean processing - ext cycle   | 115       | 129       |
| % fac's pass'g MQSA drkrm fog | 38        | 89        |
| Mean phantom obj's visible†   |           |           |
| fibers                        | 4.4       | 4.6       |
| specks                        | 3.3       | 3.8       |
| masses                        | 3.8       | 3.7       |
| Mean O. D. phantom film       | 1.13      | 1.40      |

<sup>1</sup>MQSA results are those as of 10/95

\*Mean glandular dose for 1992 was recalculated here only for comparison purposes, using same dose tables as for MQSA values of dose.

\*\*1992 NEXT used 1100 alloy al; 1995 MQSA used 1145 alloy.

†Objects are raw scores without artifact subtraction. (Artifacts were not evaluated in the 1992 NEXT survey.)